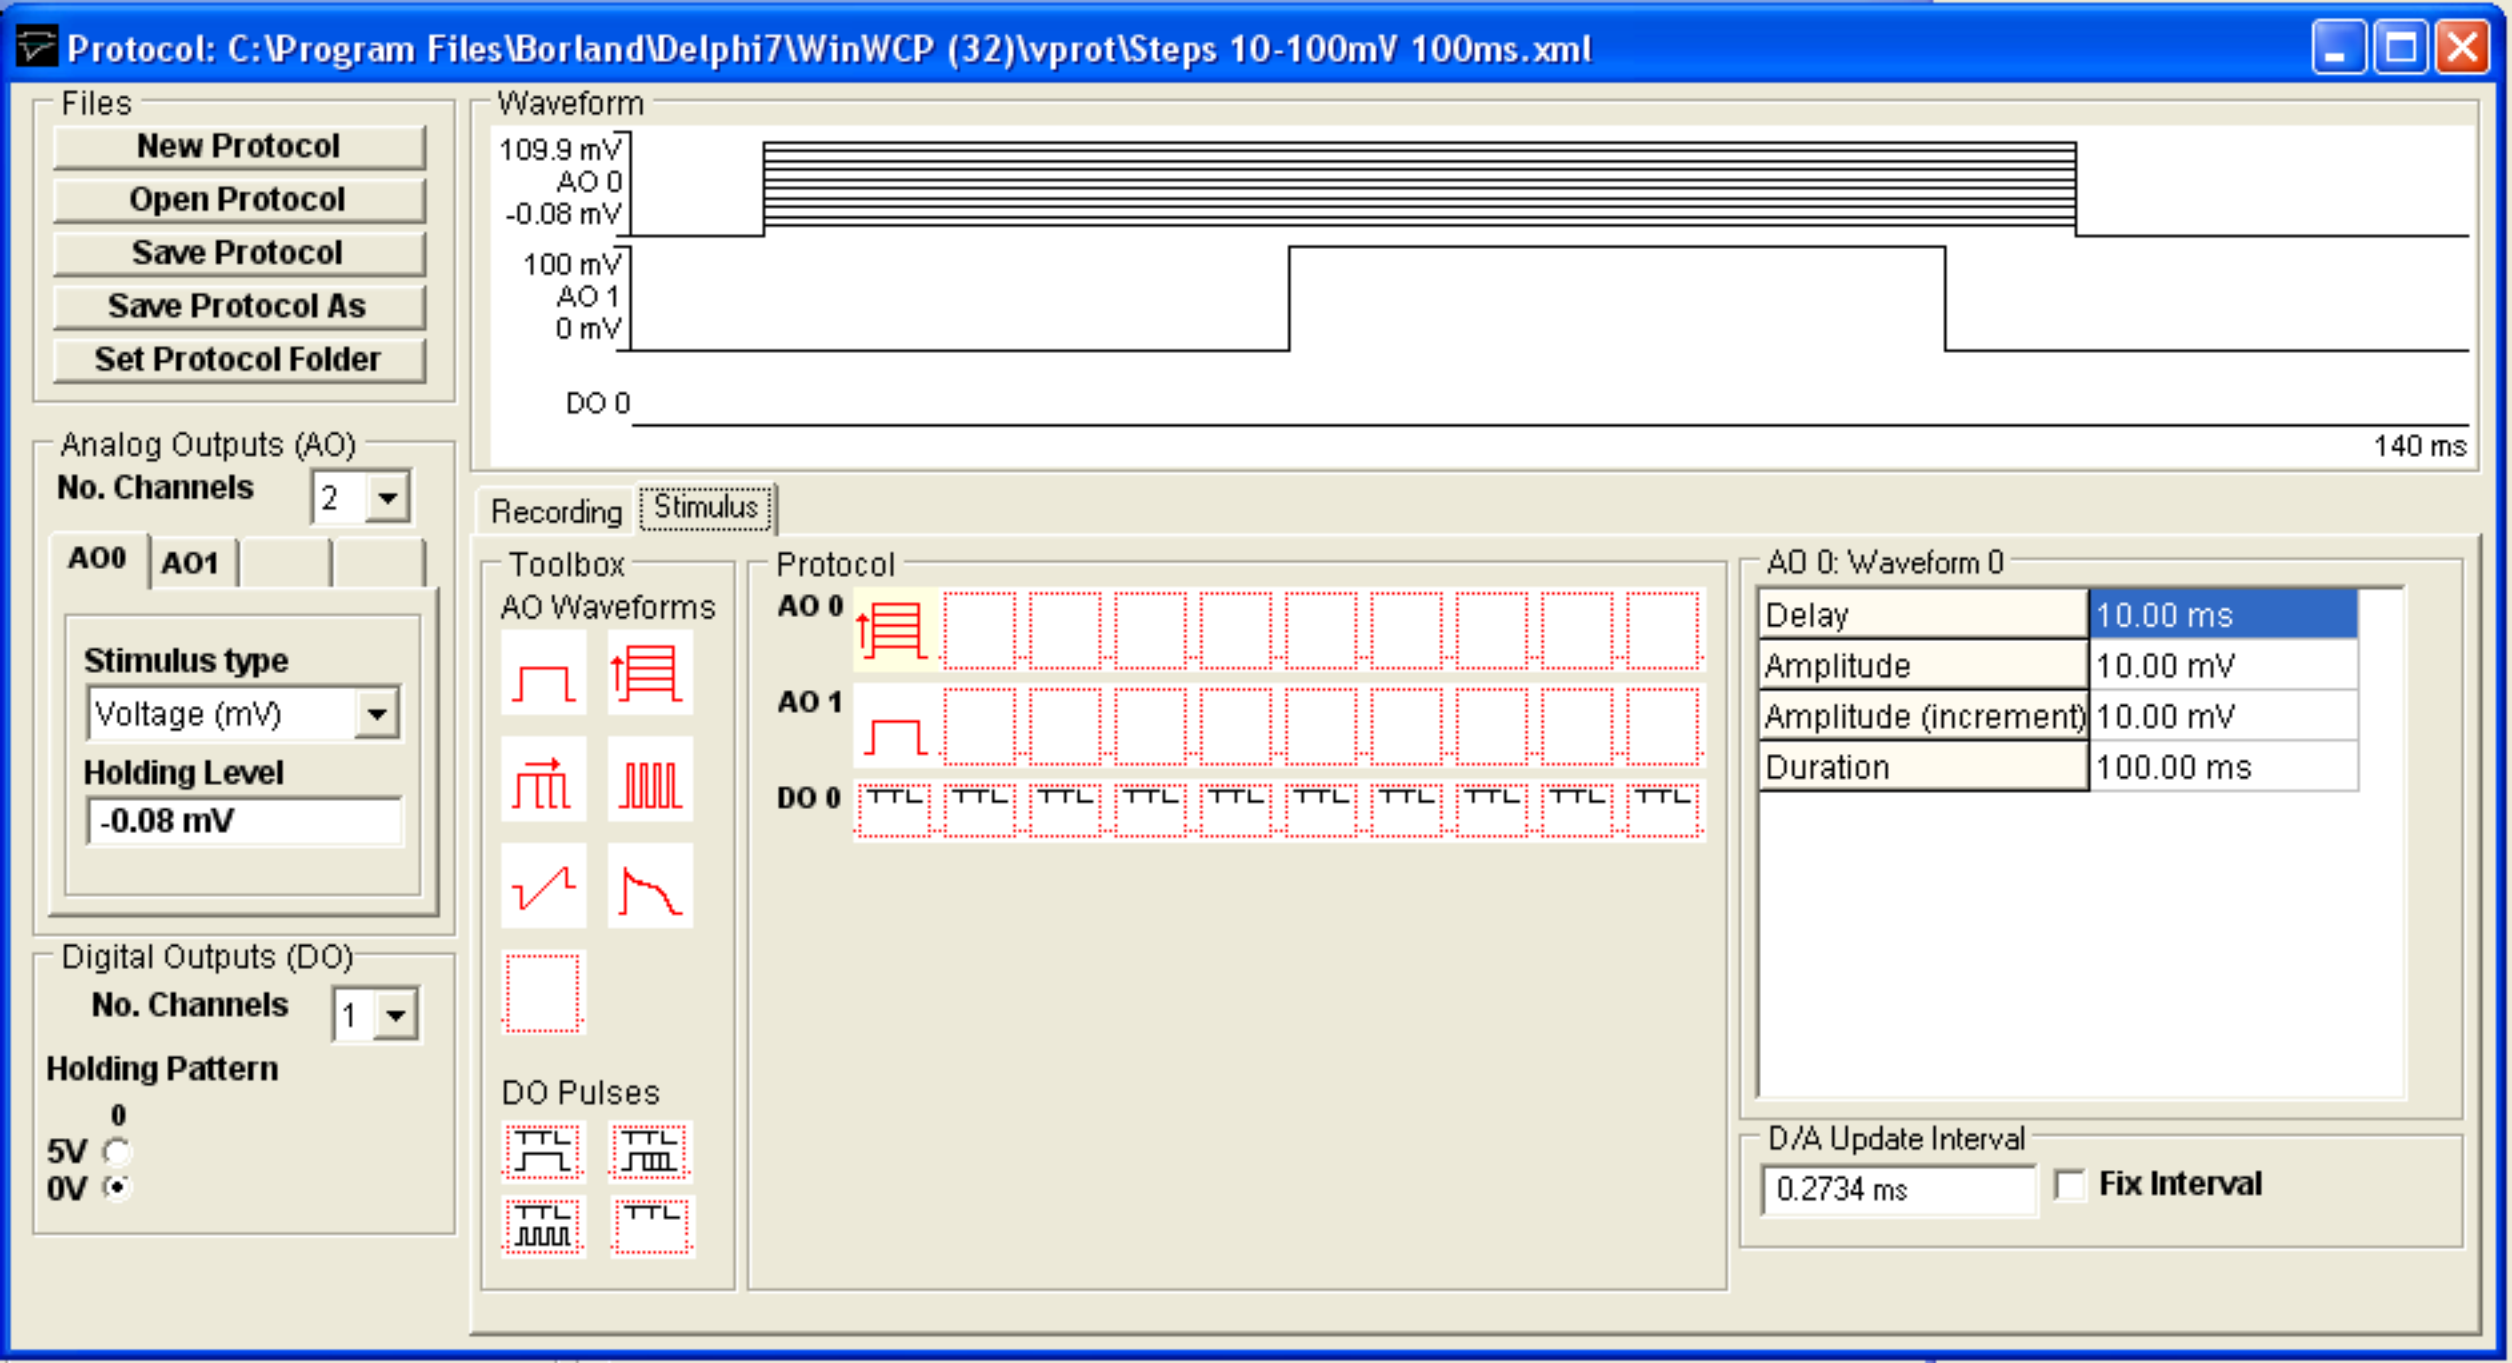

Protocol: C:\Program Files\Borland\Delphi7\WinWCP (32)\vprot\Steps 10-100mV 100ms.xml
Files
New Protocol
Open Protocol
Save Protocol
Save Protocol As
Set Protocol Folder
Analog Outputs (AO)
No. Channels
2
AO0
AO1
Stimulus type
Voltage (mV)
Holding Level
-0.08 mV
Digital Outputs (DO)
No. Channels
1
Holding Pattern
0
5V
0V
Waveform
109.9 mV
AO 0
-0.08 mV
100 mV
AO 1
0 mV
DO 0
140 ms
Recording
Stimulus
Toolbox
AO Waveforms
DO Pulses
Protocol
AO 0
AO 1
DO 0
AO 0: Waveform 0
Delay
10.00 ms
Amplitude
10.00 mV
Amplitude (increment)
10.00 mV
Duration
100.00 ms
D/A Update Interval
0.2734 ms
Fix Interval